
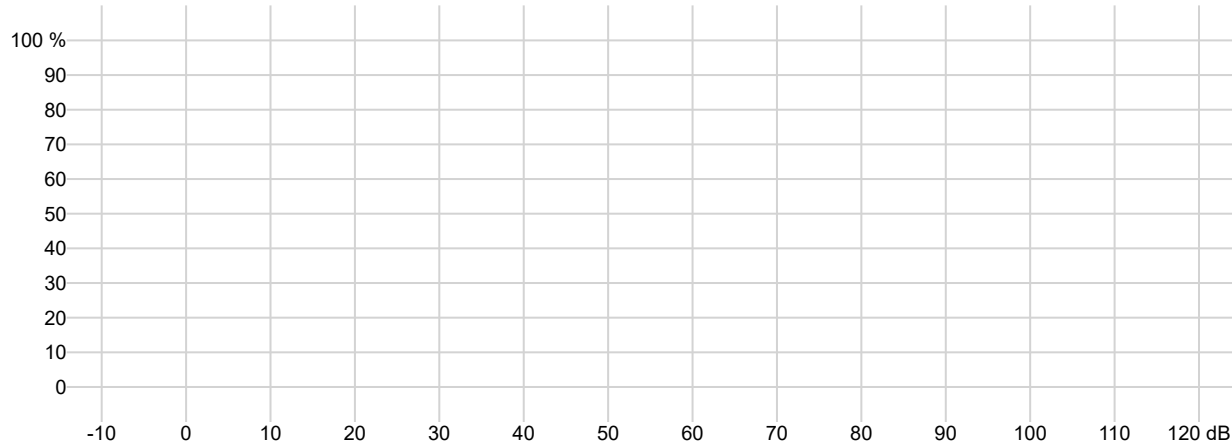
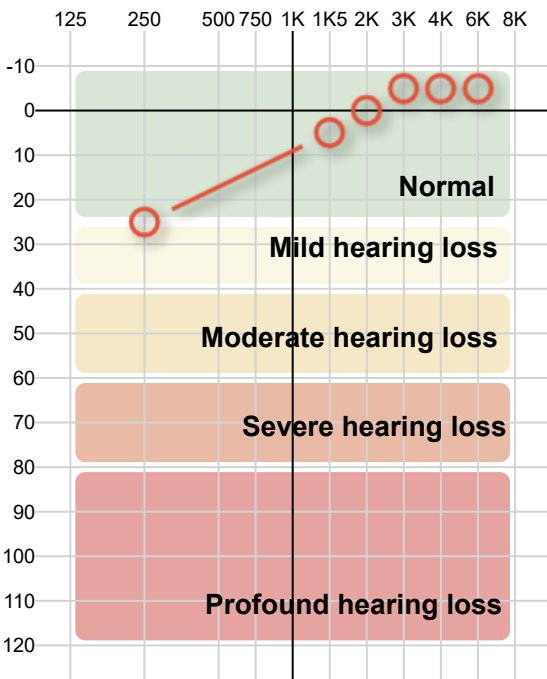


ampliSuite Patient Record

Test date : 2/23/2021

Patient	Device info	Examiner
Name : Olesen Morten	Serial no : 58595	Name : Ole Olesen
Date of Birth : 1/1/1991	Calibrated : 12/6/2018	Signed :
	Product : Otosure	
	Phones : DD45 DD45	

Left Ear											Right Ear										
125	250	500	750	1K	1K5	2K	3K	4K	6K	8K	125	250	500	750	1K	1K5	2K	3K	4K	6K	8K
-5		0		5	0	0	10	0	-5		AC		25			5	0	-5	-5	-5	
											AM										
											BC										
											BM										

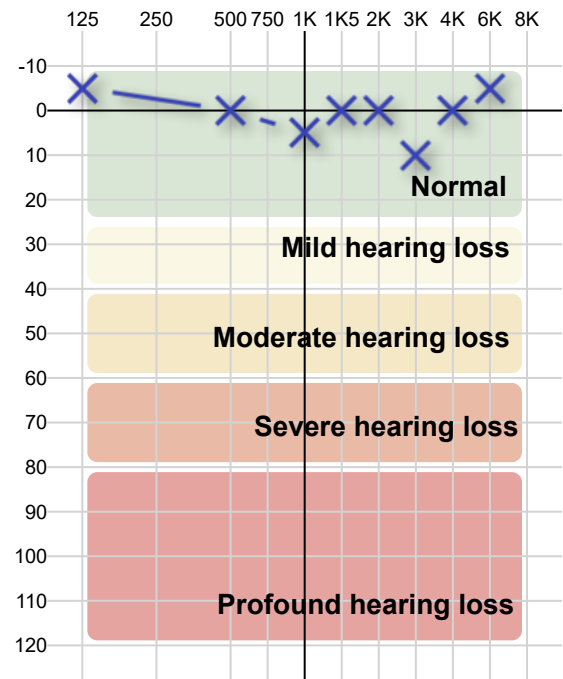

ampliSuite Patient Record**Test date : 2/23/2021**

Patient	Device info	Examiner
Name : Olesen Morten	Serial no : 58595	Name : Ole Olesen
Date of Birth : 1/1/1991	Calibrated : 12/6/2018	Signed :
	Product : Otosure	
	Phones : DD45	
	DD45	

Comments

Hørsel ok. Kalles ikke inn igjen.